

Standard Specification for Preformed Cranioplasty Plates¹

This standard is issued under the fixed designation F 452; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This specification covers preformed cranioplasty plates which do not require further alteration for covering skull defects. This specification covers compositional and physical performance and packaging requirements, but does not cover toxicity nor biocompatibility of the materials.

2. Referenced Documents

2.1 ASTM Standards:

F 56 Specification for Stainless Steel Sheet and Strip for Surgical Implants²

F 75 Specification for Cobalt-28 Chromium-6 Molybdenum Alloy Castings and Casting Alloy for Surgical Implants (UNS R30075)³

F 86 Practice for Surface Preparation and Marking of Metallic Surgical Implants³

F 139 Specification for Wrought-18 Chromium-14 Nickel-2.5 Molybdenum Stainless Steel Sheet and Strip for Surgical Implants (UNS S31673)³

2.2 American Society for Quality Control (ASQC) Standard:

C1-1968 Specifications of General Requirements for a Quality Program⁴

3. Materials

3.1 Cranioplasty plates conforming to this specification shall be fabricated from materials described in the latest issue of Specifications F 56, Grade 2, F 75, or F 139, Grade 2. The condition of the material (such as, annealed, cold finished, and so forth) should be specified in the purchase order.

4. Dimensions and Tolerances

4.1 Cranioplasty plates conforming to this specification shall be fabricated in a variety of dimensions to accommodate, without further alteration, various sized skull defects.

4.2 Shape shall be contoured so as to re-establish the normal configuration and symmetry of the skull at various anticipated sites of defect such as the parietal bosses, the inion, the brow, the linea temporalis, and so forth.

4.3 Plates shall contain multiple perforations (see Fig. 1).

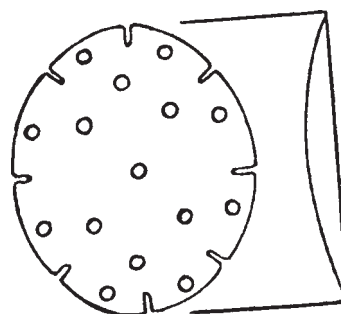


FIG. 1 Preformed Cranioplasty Plate

4.4 Thicknesses and individual shapes shall vary with need. Thickness tolerances shall be as follows:

Specified Thickness, in. (mm)	Thickness Tolerances, in. (mm)
0.005 (0.13) to 0.010 (0.25), incl	$\pm 10\%$
0.010 (0.25) to 0.020 (0.51), incl	± 0.0015 (0.04)
0.020 (0.51) to 0.035 (0.89), incl	± 0.002 (0.05)
0.035 (0.89) to 0.050 (1.27), incl	± 0.0025 (0.06)
0.050 (1.27) to 0.100 (2.54), incl	± 0.003 (0.08)

5. Finish and Identification

5.1 Cranioplasty plates conforming to this specification shall have their surfaces prepared in accordance with the latest issue of Practice F 86. Specific requirements of surface finish (if any) shall be stated in the purchase order.

5.2 The method of marking the plates shall be one of those specified in Practice F 86.

¹ This specification is under the jurisdiction of ASTM Committee F04 on Medical and Surgical Materials and Devices and is the direct responsibility of Subcommittee F04.31 on Neurosurgical Standards.

Current edition approved April 5, 1976. Published June 1976.

² Discontinued—See 1991 *Annual Book of ASTM Standards*, Vol 13.01.

³ *Annual Book of ASTM Standards*, Vol 13.01.

⁴ Available from American Society for Quality (ASQ), 600 N. Plankinton Ave., Milwaukee, WI 53203.